

Manual of Petroleum Measurement Standards Chapter 22—Testing Protocol

Section 2—Differential Pressure Flow Measurement Devices

SECOND EDITION, APRIL 2017



AMERICAN PETROLEUM INSTITUTE

Special Notes

API publications necessarily address problems of a general nature. With respect to particular circumstances, local, state, and federal laws and regulations should be reviewed.

Neither API nor any of API's employees, subcontractors, consultants, committees, or other assignees make any warranty or representation, either express or implied, with respect to the accuracy, completeness, or usefulness of the information contained herein, or assume any liability or responsibility for any use, or the results of such use, of any information or process disclosed in this publication. Neither API nor any of API's employees, subcontractors, consultants, or other assignees represent that use of this publication would not infringe upon privately owned rights.

API publications may be used by anyone desiring to do so. Every effort has been made by the Institute to assure the accuracy and reliability of the data contained in them; however, the Institute makes no representation, warranty, or guarantee in connection with this publication and hereby expressly disclaims any liability or responsibility for loss or damage resulting from its use or for the violation of any authorities having jurisdiction with which this publication may conflict.

API publications are published to facilitate the broad availability of proven, sound engineering and operating practices. These publications are not intended to obviate the need for applying sound engineering judgment regarding when and where these publications should be utilized. The formulation and publication of API publications is not intended in any way to inhibit anyone from using any other practices.

Any manufacturer marking equipment or materials in conformance with the marking requirements of an API standard is solely responsible for complying with all the applicable requirements of that standard. API does not represent, warrant, or guarantee that such products do in fact conform to the applicable API standard.

All rights reserved. No part of this work may be reproduced, translated, stored in a retrieval system, or transmitted by any means, electronic, mechanical, photocopying, recording, or otherwise, without prior written permission from the publisher. Contact the Publisher, API Publishing Services, 1220 L Street, NW, Washington, DC 20005.

Copyright © 2017 American Petroleum Institute

Foreword

Nothing contained in any API publication is to be construed as granting any right, by implication or otherwise, for the manufacture, sale, or use of any method, apparatus, or product covered by letters patent. Neither should anything contained in the publication be construed as insuring anyone against liability for infringement of letters patent.

Shall: As used in a standard, “shall” denotes a minimum requirement in order to conform to the specification.

Should: As used in a standard, “should” denotes a recommendation or that which is advised but not required in order to conform to the specification.

This document was produced under API standardization procedures that ensure appropriate notification and participation in the developmental process and is designated as an API standard. Questions concerning the interpretation of the content of this publication or comments and questions concerning the procedures under which this publication was developed should be directed in writing to the Director of Standards, American Petroleum Institute, 1220 L Street, NW, Washington, DC 20005. Requests for permission to reproduce or translate all or any part of the material published herein should also be addressed to the director.

Generally, API standards are reviewed and revised, reaffirmed, or withdrawn at least every five years. A one-time extension of up to two years may be added to this review cycle. Status of the publication can be ascertained from the API Standards Department, telephone (202) 682-8000. A catalog of API publications and materials is published annually by API, 1220 L Street, NW, Washington, DC 20005.

Suggested revisions are invited and should be submitted to the Standards Department, API, 1220 L Street, NW, Washington, DC 20005, standards@api.org.

Contents

	Page
1 Scope	1
1.1 General	1
1.2 Differential Pressure or Head-type Flow Meters	1
2 Normative References	5
3 Terms and Definitions	5
4 Field of Application	9
5 Parameter Variations Affecting Device Performance	9
5.1 Flowing Conditions	9
5.2 Meter Pipe Conditions	10
5.3 Meter Conditions	10
6 Mandatory Tests	11
6.1 Test Conditions	11
6.2 Required Piping Conditions Upstream and Downstream of the Meter	13
6.3 Test Results	13
6.4 Baseline Testing	13
6.5 Non-ideal Condition Testing (Installation Effects Testing)	14
6.6 Testing the Gas Expansion Factor for Compressible Fluids	16
6.7 Special Installation Tests	16
6.8 Testing Procedure	17
7 Test and Calibration Facility Requirements	19
7.1 Test Facility Audit Process	19
7.2 In-house Calibration Facility Verification Process	19
7.3 Test Facility Qualification	20
7.4 Validity/Precision of Test Facility Results	20
7.5 Test and Calibration Facility Uncertainty	21
8 Uncertainty and Statistical Significance Analysis and Calculation	21
8.1 Test Facility and Calibration Facility Uncertainty	21
8.2 Meter Uncertainty	21
8.3 Determination of Statistical Significance	22
9 Test Report	23
9.1 General	23
9.2 Test Facility Information	23
9.3 Calibration Facility Information	23
9.4 Meter Information	24
9.5 Description of the Full Test Matrix and Results	24
9.6 Sample Meter Test Reporting Form	25
Annex A (normative) Test Matrices for Section 6	27
Annex B (normative) Uncertainty Estimate	33
Annex C (informative) Dimensional Parameters for Prototype Testing	38
Annex D (informative) Interpolation of Uncertainty for Intermediate Area Ratios and Line Diameters	39
Bibliography	42
Figures	
1 Concentric Orifice Flow Meter	1

Contents

	Page
2 Eccentric and Segmental Orifice Flow Meters.....	2
3 Quadrant-edge and Conical Orifice Plates.....	2
4 Venturi Flow Meter.....	2
5 Flow Nozzle.....	3
6 Cone Meter.....	3
7 Dall Tube Low-loss Meter.....	3
8 Wedge Meter.....	4
9 Pitot-static Tube Meter.....	4
10 Multi-port Averaging Pitot.....	4

Introduction

This document defines a testing and reporting protocol for flow measurement devices based on the detection of a pressure differential that is created by the device in a flowing stream. The overall objectives of this testing protocol are to facilitate the introduction of new technologies, provide a standard method for validating manufacturer's performance specifications, and define the minimum requirements needed to determine relative performance characteristics of differential pressure metering devices under a standardized testing protocol. This protocol applies to both liquids and gases.

This protocol achieves these objectives by testing representative meters provided by the manufacturer in order to:

- Quantify the discharge coefficient uncertainty and the meter's sensitivity to flow profile over a range of Reynolds numbers, sizes, area ratios, upstream and downstream piping installations, and differential pressure to static pressure ratios;
- Test the gas expansion factor equation provided by the manufacturer and the manufacturer's method of determining the individual discharge coefficient for each meter to determine if they are statistically similar;
- Report the results of the testing and disclose any results that are not statistically similar as discovered during the testing process.

Performance characteristics such as discharge coefficient uncertainty, installation effects, the gas expansion factor equation, and the method of determining the discharge coefficient, can be performed as a type test under this protocol. For these characteristics, the results obtained from the tests described in this protocol can be applied to all meters of the same design that are used within the limits of the parameters tested under this protocol (e.g. size, area ratio, Reynolds number, differential pressure to static pressure ratio).

This is not a type-testing protocol for those meters that use a standard discharge coefficient equation for all meters of the same model, size, and area ratio. This standard requires the discharge coefficient or discharge coefficient equation to be determined for each individual meter. Quantifying the uncertainty of a standard discharge coefficient equation based on the statistical variation of dimensions in the manufacturing process is beyond the scope of this protocol. This protocol assumes that the influence of dimensional variation is quantified by individually testing each meter to determine its discharge coefficient under baseline conditions.

Examples of flow meters covered in this standard include, but are not limited to, orifice plates, Venturis, nozzles, cone-type meters, wedge meters, and multiport averaging Pitot tubes. However, this protocol does not cover differential devices for which an API standard has been published (the flange-tapped orifice plate per API *MPMS* Ch. 14.3, for example).

Chapter 22—Testing Protocol

Section 2—Differential Pressure Flow Measurement Devices

1 Scope

1.1 General

The testing protocol is limited to single-phase Newtonian fluid flow, and no consideration is given to pulsation effects. Further revisions of this document may include the testing of such meters in wet gas or multi-phase service and the effects of pulsation. This standard does not address testing protocols of those devices that operate on the principle of critical or choked flow condition of fluids.

The testing protocol covers any flow meter operating on the principle of a local change in flow velocity caused by the meter geometry, giving a corresponding change of pressure between two reference locations. There are several types of differential pressure meters available to industry. It is the purpose of this standard to illustrate the range of applications of each meter design and not to endorse any specific meter. The basic principle of operation of the flow measuring devices follows the physical laws relating to the conservation of energy and mass for the fluid flows through the device.

Any API *MPMS* document addressing a specific type or design of differential pressure flow measuring device will supersede the requirements of this document for that type or design. An example of such standards are all parts of API *MPMS*, Chapter 14.3, Concentric, Square-Edged Orifice Meters.

1.2 Differential Pressure or Head-type Flow Meters

The operating principle of a differential pressure flow meter is based on two physical laws - the conservation of energy and conservation of mass, where changes in flow cross-sectional area and/or flow path produce a differential pressure, which is a function of the flow velocity, fluid path, and fluid properties.

This testing protocol applies to all types of differential-pressure meters. The examples presented below illustrate some of the applicable meter designs; however, this protocol is not limited to these meter types.

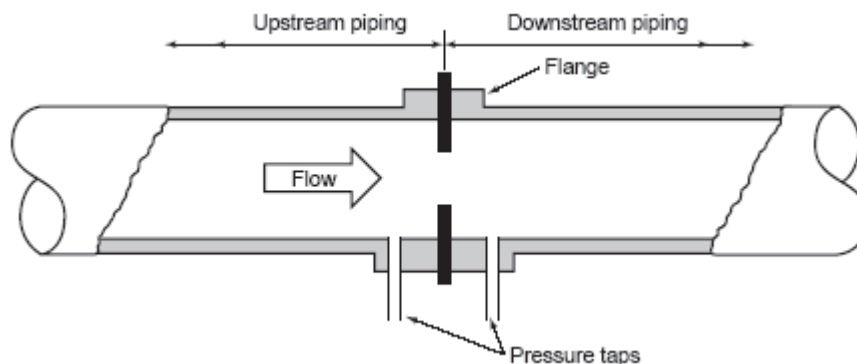


Figure 1—Concentric Orifice Flow Meter

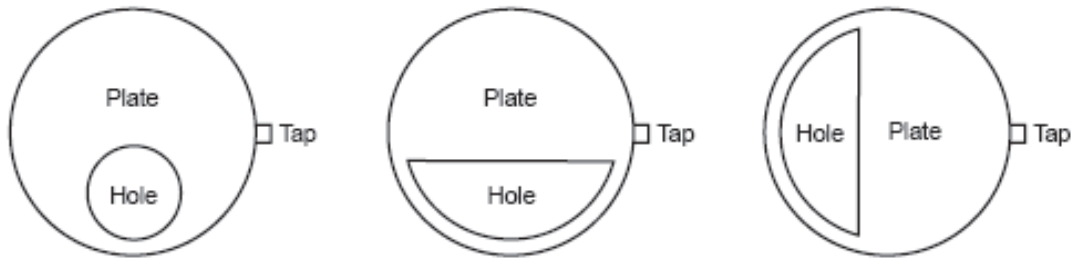


Figure 2—Eccentric and Segmental Orifice Flow Meters

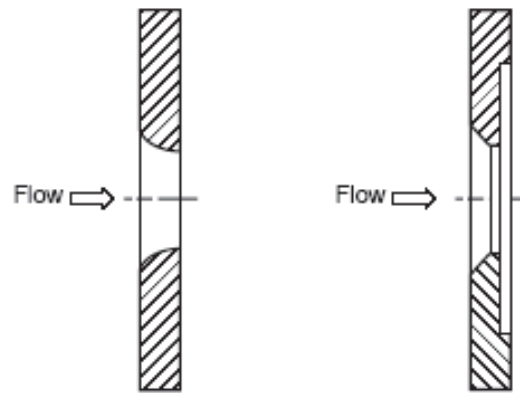


Figure 3—Quadrant-edge and Conical Orifice Plates

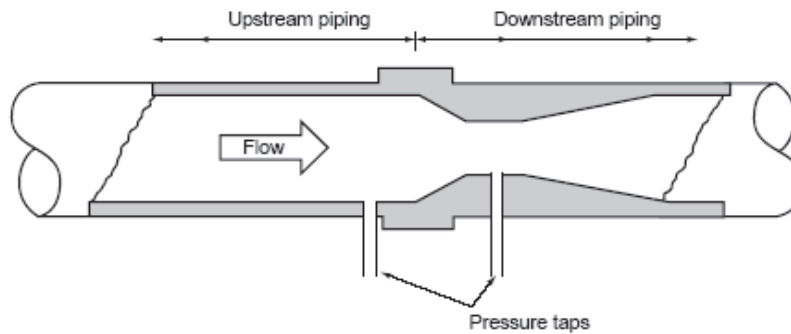


Figure 4—Venturi Flow Meter