# American National Standard

# ANSI/AAMI/ ISO 25539-3: 2011/(R)2015

Cardiovascular implants — Endovascular devices — Part 3: Vena cava filters



# Objectives and uses of AAMI standards and recommended practices

It is most important that the objectives and potential uses of an AAMI product standard or recommended practice are clearly understood. The objectives of AAMI's technical development program derive from AAMI's overall mission: the advancement of medical instrumentation. Essential to such advancement are (1) a continued increase in the safe and effective application of current technologies to patient care, and (2) the encouragement of new technologies. It is AAMI's view that standards and recommended practices can contribute significantly to the advancement of medical instrumentation, provided that they are drafted with attention to these objectives and provided that arbitrary and restrictive uses are avoided.

A voluntary standard for a medical device recommends to the manufacturer the information that should be provided with or on the product, basic safety and performance criteria that should be considered in qualifying the device for clinical use, and the measurement techniques that can be used to determine whether the device conforms with the safety and performance criteria and/or to compare the performance characteristics of different products. Some standards emphasize the information that should be provided with the device, including performance characteristics, instructions for use, warnings and precautions, and other data considered important in ensuring the safe and effective use of the device in the clinical environment. Recommending the disclosure of performance characteristics often necessitates the development of specialized test methods to facilitate uniformity in reporting; reaching consensus on these tests can represent a considerable part of committee work. When a drafting committee determines that clinical concerns warrant the establishment of minimum safety and performance criteria, referee tests must be provided and the reasons for establishing the criteria must be documented in the rationale.

A *recommended practice* provides guidelines for the use, care, and/or processing of a medical device or system. A recommended practice does not address device performance *per se*, but rather procedures and practices that will help ensure that a device is used safely and effectively and that its performance will be maintained.

Although a device standard is primarily directed to the manufacturer, it may also be of value to the potential purchaser or user of the device as a frame of reference for device evaluation. Similarly, even though a recommended practice is usually oriented towards healthcare professionals, it may be useful to the manufacturer in better understanding the environment in which a medical device will be used. Also, some recommended practices, while not addressing device performance criteria, provide guidelines to industrial personnel on such subjects as sterilization processing, methods of collecting data to establish safety and efficacy, human engineering, and other processing or evaluation techniques; such guidelines may be useful to health care professionals in understanding industrial practices.

In determining whether an AAMI standard or recommended practice is relevant to the specific needs of a potential user of the document, several important concepts must be recognized:

All AAMI standards and recommended practices are *voluntary* (unless, of course, they are adopted by government regulatory or procurement authorities). The application of a standard or recommended practice is solely within the discretion and professional judgment of the user of the document.

Each AAMI standard or recommended practice reflects the collective expertise of a committee of health care professionals and industrial representatives, whose work has been reviewed nationally (and sometimes internationally). As such, the consensus recommendations embodied in a standard or recommended practice are intended to respond to clinical needs and, ultimately, to help ensure patient safety. A standard or recommended practice is limited, however, in the sense that it responds generally to perceived risks and conditions that may not always be relevant to specific situations. A standard or recommended practice is an important *reference* in responsible decision-making, but it should never *replace* responsible decision-making.

Despite periodic review and revision (at least once every five years), a standard or recommended practice is necessarily a static document applied to a dynamic technology. Therefore, a standards user must carefully review the reasons why the document was initially developed and the specific rationale for each of its provisions. This review will reveal whether the document remains relevant to the specific needs of the user.

Particular care should be taken in applying a product standard to existing devices and equipment, and in applying a recommended practice to current procedures and practices. While observed or potential risks with existing equipment typically form the basis for the safety and performance criteria defined in a standard, professional judgment must be used in applying these criteria to existing equipment. No single source of information will serve to identify a particular product as "unsafe". A voluntary standard can be used as one resource, but the ultimate decision as to product safety and efficacy must take into account the specifics of its utilization and, of course, cost-benefit considerations. Similarly, a recommended practice should be analyzed in the context of the specific needs and resources of the individual institution or firm. Again, the rationale accompanying each AAMI standard and recommended practice is an excellent guide to the reasoning and data underlying its provision.

In summary, a standard or recommended practice is truly useful only when it is used in conjunction with other sources of information and policy guidance and in the context of professional experience and judgment.

# INTERPRETATIONS OF AAMI STANDARDS AND RECOMMENDED PRACTICES

Requests for interpretations of AAMI standards and recommended practices must be made in writing, to the AAMI Vice President, Standards Policy and Programs. An official interpretation must be approved by letter ballot of the originating committee and subsequently reviewed and approved by the AAMI Standards Board. The interpretation will become official and representation of the Association only upon exhaustion of any appeals and upon publication of notice of interpretation in the "Standards Monitor" section of the AAMI News. The Association for the Advancement of Medical Instrumentation disclaims responsibility for any characterization or explanation of a standard or recommended practice which has not been developed and communicated in accordance with this procedure and which is not published, by appropriate notice, as an official interpretation in the AAMI News.

# Cardiovascular implants — Endovascular devices — Part 3: Vena cava filters

Approved 30 November 2011 by Association for the Advancement of Medical Instrumentation

Approved 5 June 2012 and reaffirmed 24 November 2015 by American National Standards Institute

**Abstract:** Specifies requirements for vena cava filters, based upon current medical knowledge. With regard to safety, it gives requirements for intended performance, design attributes, materials, design evaluation, manufacturing, sterilization, packaging and information supplied by the manufacturer. It should be considered as a supplement to ISO 14630, which specifies general requirements for the performance of non-active surgical implants.

Keywords: clinical, delivery, design, dilator, evaluation, IVC, materials, performance, reporting, sampling, sheath

# **AAMI Standard**

This Association for the Advancement of Medical Instrumentation (AAMI) standard implies a consensus of those substantially concerned with its scope and provisions. The existence of an AAMI standard does not in any respect preclude anyone, whether they have approved the standard or not, from manufacturing, marketing, purchasing, or using products, processes, or procedures not conforming to the standard. AAMI standards are subject to periodic review, and users are cautioned to obtain the latest editions.

**CAUTION NOTICE:** This AAMI standard may be revised or withdrawn at any time. AAMI procedures require that action be taken to reaffirm, revise, or withdraw this standard no later than 5 years from the date of publication. Interested parties may obtain current information on all AAMI standards by calling or writing AAMI, or by visiting the AAMI website at <u>www.aami.org</u>.

All AAMI standards, recommended practices, technical information reports, and other types of technical documents developed by AAMI are *voluntary*, and their application is solely within the discretion and professional judgment of the user of the document. Occasionally, voluntary technical documents are adopted by government regulatory agencies or procurement authorities, in which case the adopting agency is responsible for enforcement of its rules and regulations.

Published by

Association for the Advancement of Medical Instrumentation 4301 N. Fairfax Drive, Suite 301 Arlington, VA 22203-1633 www.aami.org

© 2012 by the Association for the Advancement of Medical Instrumentation

#### All Rights Reserved

This publication is subject to copyright claims of ISO, ANSI, and AAMI. No part of this publication may be reproduced or distributed in any form, including an electronic retrieval system, without the prior written permission of AAMI. All requests pertaining to this document should be submitted to AAMI. It is illegal under federal law (17 U.S.C. § 101, et seq.) to make copies of all or any part of this document (whether internally or externally) without the prior written permission of the Association for the Advancement of Medical Instrumentation. Violators risk legal action, including civil and criminal penalties, and damages of \$100,000 per offense. For permission regarding the use of all or any part of this document, complete the reprint request form at <a href="http://www.aami.org">www.aami.org</a> or contact AAMI at 4301 N. Fairfax Drive, Suite 301, Arlington, VA 22203-1633. Phone: +1-703-525-4890; Fax: +1-703-525-1067.

Printed in the United States of America

ISBN 1-57020-443-8

# Contents

Glossa	ry of equivalent standards	. v
Commi	ttee Representation	vii
Backgr	ound of ANSI/AAMI adoption of ISO 25539-3:2011	/iii
Forewo	ord	ix
Introdu	iction	X
1	Scope	. 1
2	Normative references	. 1
3	Terms and definitions	. 2
4 4.1 4.2	General requirements Classification Size	. 5
5	Intended performance	. 5
6 6.1 6.2 6.3 6.4 6.5 6.6 6.7 6.8 7	Design attributes General Sheath/dilator kit for endovascular filter system Filter system Filter Optional filter Sheath/dilator kit for endovascular retrieval/conversion system Retrieval/conversion system Endovascular systems Materials	5 6 6 6 6 7
8 8.1 8.2 8.3 8.4 8.5 8.6 8.7	Design evaluation General	7 8 8 9 25
9	Post-market surveillance	34
10	Manufacturing	34
11 11.1 11.2 11.3	Sterilization Products supplied sterile Products supplied non-sterile Sterilization residuals	34 35
12 12.1 12.2 12.3	Packaging Protection from damage in storage and transport Marking Information supplied by the manufacturer	35 36

Annex A (informative) Attributes of endovascular devices — Vena cava filters — Technical and clinical considerations	39
Annex B (informative) Descriptions of potential device effects of failure and failure modes and descriptions of detrimental clinical effects	53
Annex C (informative) Bench and analytical tests	58
Annex D (informative) Test methods	62
Annex E (informative) Examples of terms for clinical use of vena cava filters	92
Bibliography	94

## **Glossary of equivalent standards**

International Standards adopted in the United States may include normative references to other International Standards. For each International Standard that has been adopted by AAMI (and ANSI), the table below gives the corresponding U.S. designation and level of equivalency to the International Standard. NOTE: Documents are sorted by international designation. The code in the US column, "(R)20xx" indicates the year the document was officially reaffirmed by AAMI. E.g., ANSI/AAMI/ISO 10993-4:2002/(R)2009 indicates that 10993-4, originally approved and published in 2002, was reaffirmed without change in 2009.

Other normatively referenced International Standards may be under consideration for U.S. adoption by AAMI; therefore, this list should not be considered exhaustive.

International designation	U.S. designation	Equivalency
IEC 60601-1:2005	ANSI/AAMI ES60601-1:2005/(R)2012 and	Major technical variations
Technical Corrigendum 1 and 2	ANSI/AAMI ES60601-1:2005/A2:2010/(R)2012	
	ANSI/AAMI ES60601-1:2005/C1:2009/(R)2012 (amdt)	C1 Identical to Corrigendum 1
	(and)	& 2
IEC 60601-1-11:2010	ANSI/AAMI HA60601-1-11:2011	Major technical variations
IEC 60601-1-2:2007	ANSI/AAMI/IEC 60601-1-2:2007/(R)2012	Identical
IEC 60601-2-2:2009	ANSI/AAMI/IEC 60601-2-2:2009	Identical
IEC 60601-2-4:2010	ANSI/AAMI/IEC 60601-2-4:2010	Identical
IEC 60601-2-16:2008	ANSI/AAMI/IEC 60601-2-16:2008	Identical
IEC 60601-2-19:2009 IEC 60601-2-20:2009	ANSI/AAMI/IEC 60601-2-19:2009 ANSI/AAMI/IEC 60601-2-20:2009	Identical
IEC 60601-2-20.2009	ANSI/AAMI/IEC 60601-2-20.2009 ANSI/AAMI/IEC 60601-2-21:2009	Identical Identical
IEC 60601-2-21:2009 IEC 60601-2-24:1998	ANSI/AAMI ID26:2004/(R)2009	Major technical variations
IEC 60601-2-25:2011	ANSI/AAMI/IEC 60601-2-25:2011	Identical
IEC 60601-2-27:2011	ANSI/AAMI/IEC 60601-2-27:2011	Identical
IEC 60601-2-47:2001	ANSI/AAMI EC38:2007	Major technical variations
IEC 60601-2-50:2009	ANSI/AAMI/IEC 60601-2-50:2009	Identical
IEC 80001-1:2010	ANSI/AAMI/IEC 80001-1:2010	Identical
IEC 80601-2-30:2009 and Technical	ANSI/AAMI/IEC 80601-2-30:2009 and ANSI/AAMI/IEC 80601-2-30:2009/C1:2009 (amdt)	Identical (with inclusion) C1 Identical to Corrigendum 1
Corrigendum 1	ANSI/AAMI/IEC 80601-2-30:2009/C1:2009 (amdt)	C1 Identical to Corrigendum 1
IEC 80601 2 58:2008	– consolidated text ANSI/AAMI/IEC 80601-2-58:2008	Identical
IEC 80601-2-58:2008 IEC/TR 60878:2009	ANSI/AAMI/IEC 80001-2-38.2008 ANSI/AAMI/IEC TIR60878:2003	Identical
IEC/TR 61289:2011	ANSI/AAMI/IEC TIR61289:2011	Identical
IEC/TR 62296:2009	ANSI/AAMI/IEC TIR62296:2009	Identical
IEC 62304:2006	ANSI/AAMI/IEC 62304:2006	Identical
IEC/TR 62348:2006	ANSI/AAMI/IEC TIR62348:2006	Identical
IEC/TR 62354:2009	ANSI/AAMI/IEC TIR62354:2009	Identical
IEC 62366:2007	ANSI/AAMI/IEC 62366:2007	Identical
IEC/TR 80002-1:2009	ANSI/IEC/TR 80002-1:2009	Identical
ISO 5840:2005	ANSI/AAMI/ISO 5840:2005/(R)2010	Identical
ISO 7198:1998	ANSI/AAMI/ISO 7198:1998/2001/(R)2010	Identical
ISO 7199:2009 and Amendment 1:2012	ANSI/AAMI/ISO 7199:2009 and Amendment 1:2012	Identical
ISO 8637:2010	AMERICIANI ANNI/ISO 8637:2010	Identical
ISO 8638:2010	ANSI/AAMI/ISO 8638:2010	Identical
ISO 10993-1:2009	ANSI/AAMI/ISO 10993-1:2009	Identical
ISO 10993-2:2006	ANSI/AAMI/ISO 10993-2:2006/(R)2010	Identical
ISO 10993-3:2003	ANSI/AAMI/ISO 10993-3:2003/(R)2009	Identical
ISO 10993-4:2002 and	ANSI/AAMI/ISO 10993-4:2002/(R)2009 and Amendment 1:2006/(R)2009	Identical
Amendment 1:2006		
ISO 10993-5:2009	ANSI/AAMI/ISO 10993-5:2009	Identical
ISO 10993-6:2007	ANSI/AAMI/ISO 10993-6:2007/(R)2010	Identical
ISO 10993-7:2008 ISO 10993-9:2009	ANSI/AAMI/ISO 10993-7:2008/(R)2012 ANSI/AAMI/ISO 10993-9:2009	Identical
ISO 10993-0:2009	ANSI/AAMI/ISO 10993-9:2009 ANSI/AAMI/ISO 10993-10:2010	Identical Identical
ISO 10993-11:2006	ANSI/AAMI/ISO 10993-10:2010 ANSI/AAMI/ISO 10993-11:2006/(R)2010	Identical
ISO 10993-12:2012	ANSI/AAMI/ISO 10993-12:2012	Identical
ISO 10993-13:2010	ANSI/AAMI/ISO 10993-13:2010	Identical
ISO 10993-14:2001	ANSI/AAMI/ISO 10993-14:2001/(R)2006	Identical
ISO 10993-15:2000	ANSI/AAMI/ISO 10993-15 2000/(R)2006	Identical
ISO 10993-16:2010	ANSI/AAMI/ISO 10993-16:2010	Identical
	ANSI/AAMI/ISO 10993-17:2002/(R)2008	Identical
ISO 10993-17:2002		
ISO 10993-18:2005	ANSI/AAMI BE83:2006/(R)2011	Major technical variations
ISO 10993-18:2005 ISO/TS 10993-19:2006	ANSI/AAMI BE83:2006/(R)2011 ANSI/AAMI/ISO TIR10993-19:2006	Identical
ISO 10993-18:2005	ANSI/AAMI BE83:2006/(R)2011	

© 2012 Association for the Advancement of Medical Instrumentation 
ANSI/AAMI/ISO 25539-3:2011

International designation	U.S. designation	Equivalency
ISO 11137-1:2006	ANSI/AAMI/ISO 11137-1:2006/(R)2010	Identical
ISO 11137-2:2012	ANSI/AAMI/ISO 11137-2:2012	Identical
ISO 11137-3:2006 ISO 11138-1:2006	ANSI/AAMI/ISO 11137-3:2006/(R)2010 ANSI/AAMI/ISO 11138-1:2006/(R)2010	Identical Identical
ISO 11138-2:2006	ANSI/AAMI/ISO 11138-2:2006/(R)2010	Identical
ISO 11138-3:2006	ANSI/AAMI/ISO 11138-3:2006/(R)2010	Identical
ISO 11138-4:2006	ANSI/AAMI/ISO 11138-4:2006/(R)2010	Identical
ISO 11138-5:2006 ISO/TS 11139:2006	ANSI/AAMI/ISO 11138-5:2006/(R)2010 ANSI/AAMI/ISO 11139:2006	Identical Identical
ISO 11140-1:2005	ANSI/AAMI/ISO 11133.2000 ANSI/AAMI/ISO 11140-1:2005/(R)2010	Identical
ISO 11140-3:2007	ANSI/AAMI/ISO 11140-3:2007	Identical
ISO 11140-4:2007	ANSI/AAMI/ISO 11140-4:2007	Identical
ISO 11140-5:2007 ISO 11607-1:2006	ANSI/AAMI/ISO 11140-5:2007 ANSI/AAMI/ISO 11607-1:2006/(R)2010	Identical Identical
ISO 11607-1.2006	ANSI/AAMI/ISO 11607-1.2006/(R)2010 ANSI/AAMI/ISO 11607-2:2006/(R)2010	Identical
ISO 11663:2009	ANSI/AAMI/ISO 11633:2009	Identical
ISO 11737-1:2006	ANSI/AAMI/ISO 11737-1:2006	Identical
ISO 11737-2:2009	ANSI/AAMI/ISO 11737-2:2009	Identical
ISO/TS 12417:2011 ISO 13022:2012	ANSI/AAMI/ISO TIR12417:2011 ANSI/AAMI/ISO 13022:2012	Identical Identical
ISO 13408-1:2008	ANSI/AAMI/ISO 13408-1:2008/(R)2011	Identical
ISO 13408-2:2003	ANSI/AAMI/ISO 13408-2:2003	Identical
ISO 13408-3:2006	ANSI/AAMI/ISO 13408-3:2006	Identical
ISO 13408-4:2005 ISO 13408-5:2006	ANSI/AAMI/ISO 13408-4:2005 ANSI/AAMI/ISO 13408-5:2006	Identical Identical
ISO 13408-6:2006	ANSI/AAMI/ISO 13408-6:2006	Identical
ISO 13408-7:20121	ANSI/AAMI/ISO 13408-7:2012	Identical
ISO 13485:2003	ANSI/AAMI/ISO 13485:2003/(R)2009	Identical
ISO 13958:2009 ISO 13959:2009	ANSI/AAMI/ISO 13958:2009 ANSI/AAMI/ISO 13959:2009	Identical Identical
ISO 13959.2009	ANSI/AAMI/ISO 13959.2009 ANSI/AAMI/ISO 14155:2011	Identical
ISO 14160:2011	ANSI/AAMI/ISO 14160:2011	Identical
ISO 14161:2009	ANSI/AAMI/ISO 14161:2009	Identical
ISO 14708-3:2008	ANSI/AAMI/ISO 14708-3:2008	Identical
ISO 14708-4:2008 ISO 14708-5:2010	ANSI/AAMI/ISO 14708-4:2008 ANSI/AAMI /ISO 14708-5:2010	Identical Identical
ISO 14937:2009	ANSI/AAMI/ISO 14937:2009	Identical
ISO/TR 14969:2004	ANSI/AAMI/ISO TIR14969:2004	Identical
ISO 14971:2007	ANSI/AAMI/ISO 14971:2007/(R)2010	Identical
ISO 15223-1:2007 and A1:2008	ANSI/AAMI/ISO 15223-1:2007/(R)2012 and A1:2008/(R)2012	Identical
ISO 15223-2:2010	ANSI/AAMI/ISO 15223-2:2010	Identical
ISO 15225:2010	ANSI/AAMI/ISO 15225:2010	Identical
ISO 15674:2009	ANSI/AAMI/ISO 15674:2009	Identical
ISO 15675:2009 ISO 15882:2008	ANSI/AAMI/ISO 15675:2009 ANSI/AAMI/ISO 15882:2008	Identical Identical
ISO 15883-1:2006	ANSI/AAMI ST15883-1:2009	Major technical variations
ISO/TR 16142:2006	ANSI/AAMI/ISO TIR16142:2005	Identical
ISO 17664:2004	ANSI/AAMI ST81:2004	Major technical variations
ISO 17665-1:2006 ISO/TS 17665-2:2009	ANSI/AAMI/ISO 17665-1:2006 ANSI/AAMI/ISO TIR17665-2:2009	Identical (with inclusions)
ISO 18472:2006	ANSI/AAMI/ISO 11(1/003-2.2009 ANSI/AAMI/ISO 18472:2006/(R)2010	Identical
ISO/TS 19218-1:2011	ANSI/AAMI/ISO TIR19218:2011	Identical
ISO 20857:2010	ANSI/AAMI/ISO 20857:2010	Identical
ISO 22442-1:2007 ISO 22442-2:2007	ANSI/AAMI/ISO 22442-1:2007 ANSI/AAMI/ISO 22442-2:2007	Identical Identical
ISO 22442-3:2007	ANSI/AAMI/ISO 22442-2.2007 ANSI/AAMI/ISO 22442-3:2007	Identical
ISO/TR 22442-4:2010	ANSI/AAMI/ISO TIR22442-4:2010	Identical
ISO 23500:2011	ANSI/AAMI/ISO 23500:2011	Identical
ISO/TS 23810:2012 ISO 25539-1:2003 and A1:2005	ANSI/AAMI/ISO TIR23810:2012 ANSI/AAMI/ISO 25539-1:2003/(R)2009 and	Identical Identical
130 20039-1.2003 dru A1.2003	ANSI/AAMI/ISO 25539-1:2003/(R)2009 and A1:2005/(R)2009	
ISO 25539-2:2008	ANSI/AAMI/ISO 25539-2:2008	Identical
ISO 25539-3:2011	ANSI/AAMI/ISO 25539-3:2011	Identical
ISO 26722:2009	ANSI/AAMI/ISO 26722:2009	Identical
ISO 27185:2012 ISO 27186:2010	ANSI/AAMI/ISO 27185:2012 ANSI/AAMI/ISO 27186:2010	Identical Identical
ISO 80369-1:2010	ANSI/AAMI/ISO 27180.2010 ANSI/AAMI/ISO 80369-1:2010	Identical
ISO 81060-1:2007	ANSI/AAMI/ISO 81060-1:2007	Identical
ISO 81060-2:2009	ANSI/AAMI/ISO 81060-2:2009	Identical

<sup>&</sup>lt;sup>1</sup> In production

# **Committee representation**

#### Association for the Advancement of Medical Instrumentation

#### **Vascular Prostheses Committee**

The adoption of ISO 25539-3:2011 as an American National Standard was initiated by the AAMI Vascular Prostheses Committee. The AAMI Vascular Prostheses Committee also functions as the U.S. Technical Advisory Group to the relevant work in the International Organization for Standardization (ISO). U.S. representatives from the AAMI Vascular Prostheses Committee (U.S. Sub-TAG for ISO/TC 150/SC 2/WG 3) played an active part in developing the ISO standard.

At the time this document was published, the **AAMI Vascular Prostheses Committee** (U.S. Sub-TAG for ISO/TC 150/SC 2/WG 3) had the following members:

Cochairs	Richard Bianco Brian Hudson
Members	Dorothy Abel, FDA/CDRH Richard Bianco, University of Minnesota Brian Choules, PhD, Med Institute, Inc. James Conti, PhD, Dynatek Dalta Scientific Instruments Jeff Elkins, Aptus Endosystems Michael Hallisey, MD, Jefferson Radiology Mark Hoekwater, Medtronic Cardiovascular Brian Hudson, Bard Peripheral Vascular Division Jason Humphrey, Boston Scientific Martin King, PhD, Hopital Saint Francois D'Assise/Quebec Biomaterials Institute Evan Lipsitz, MD, Montefiore Medical Center Lito Mejia, Bose Corporation Keith Morel, DEKRA Ning Pan, Johnson & Johnson/Ethicon Endo-Surgery Santosh Prabhu, PhD, Abbott Laboratories David Rosenthal, MD, Atlanta Vascular Specialists Louis Smith, WL Gore & Associates Ann Tunstall, PhD, SciLucent LLC Matthew Waninger, PhD, Cook, Inc. Craig Weinberg, PhD, Biomedical Device Consultants & Laboratories Robert Whirley, PhD, TriVascular Inc. Rodney White, MD, Harbor-UCLA Medical Center Christopher Zarins, MD, Stanford University Hospital
Alternates	Yolanda Bolanos, Johnson & Johnson/Cordis Corporation Lee Bolduc, Aptus Endosystems Jason Bowe, Med Institute, Inc. Jennifer Goode, FDA/CDRH Thomas Herbst, PhD, Boston Scientific Elaine Strope, PhD, Dynatek Dalta Scientific Instruments Matthew Thompson, Bose Corporation Steven Weinberg, PhD, Biomedical Device Consultants & Laboratories Michael Wolf, Medtronic Inc.

NOTE—Participation by federal agency representatives in the development of this standard does not constitute endorsement by the federal government or any of its agencies.

# Background of AAMI adoption of ISO 25539-3:2011

As indicated in the foreword to the main body of this document (page ix), the International Organization for Standardization (ISO) is a worldwide federation of national standards bodies. The United States is one of the ISO members that took an active role in the development of this standard, which was developed by ISO Technical Committee (TC) 150 Subcommittee (SC) 2, *Cardiovascular implants and extracorporeal systems,* to specify requirements for intended performance, design attributes, materials, design evaluation, manufacturing, sterilization, packaging and information supplied by the manufacturer for vena cava filters.

U.S. participation in this ISO SC is organized through the U.S. Technical Advisory Group for ISO/TC 150/SC 2, administered by the Association for the Advancement of Medical Instrumentation (AAMI).

AAMI encourages its committees to harmonize their work with international standards as much as possible. ANSI/AAMI/ISO 25539-3 was approved by the AAMI Standards Board on 30 November 2011. The AAMI Vascular Prostheses Committee (U.S. Sub-TAG for ISO/TC 150/SC 2/WG 3, Vascular prostheses) initiated the U.S. adoption of ISO 25539-3.

AAMI (and ANSI) have adopted other ISO standards. See the Glossary of Equivalent Standards for a list of ISO standards adopted by AAMI which gives the corresponding U.S. designation and the level of equivalency with the ISO standard.

As used within the context of this document, "shall" indicates requirements strictly to be followed to conform to the standard. "Should" indicates that among several possibilities, one is recommended as particularly suitable, without mentioning or excluding others, or that a certain course of action is preferred but not necessarily required, or that (in the negative form) a certain possibility or course of action should be avoided but is not prohibited. "May" is used to indicate that a course of action is permissible within the limits of the standard. "Can" is used as a statement of possibility and capability. Finally, "must" is used only to describe "unavoidable" situations, including those mandated by government regulation.

The concepts incorporated in this standard should not be considered inflexible or static. This standard, like any other, must be reviewed and updated periodically to assimilate progressive technological developments. To remain relevant, it must be modified as technological advances are made and as new data come to light.

Suggestions for improving this standard are invited. Comments and suggested revisions should be sent to Standards Department, AAMI, 4301 N. Fairfax Drive, Suite 301, Arlington, VA 22203-1633.

NOTE—Beginning with the ISO foreword on page ix, this American National Standard is identical to ISO 25539-3:2011.

# Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 25539-3 was prepared by Technical Committee ISO/TC 150, *Implants for surgery*, Subcommittee SC 2, *Cardiovascular implants and extracorporeal systems*.

ISO 25539 consists of the following parts, under the general title *Cardiovascular implants* — *Endovascular devices*:

- Part 1: Endovascular prostheses
- Part 2: Vascular stents
- Part 3: Vena cava filters

# Introduction

This part of ISO 25539 provides minimum requirements for endovascular devices and the methods of test that will enable their evaluation. It is derived from ISO/TS 15539, which serves as a rationale for its requirements. ISO/TS 15539 was developed by first identifying the design requirements for these devices and listing the potential failure modes and potential device and detrimental clinical effects. Tests were then identified to address each of the failure modes. The requirements specified in this part of ISO 25539 are based on that assessment.

# Cardiovascular implants — Endovascular devices — Part 3: Vena cava filters

### 1 Scope

This part of ISO 25539 specifies requirements for vena cava filters, based upon current medical knowledge. With regard to safety, it gives requirements for intended performance, design attributes, materials, design evaluation, manufacturing, sterilization, packaging and information supplied by the manufacturer. This part of ISO 25539 supplements ISO 14630, which specifies general requirements for the performance of non-active surgical implants.

The following are within the scope of this part of ISO 25539:

- vena cava filters used to prevent pulmonary embolism by mechanical filtration in the inferior vena cava (IVC). While this part of ISO 25539 might be useful with respect to filters implanted in other venous locations (e.g. superior vena cava, iliac veins), it does not specifically address use of filters in other implantation sites;
- sheath/dilator kits, providing that they comprise an integral component of the access, delivery or retrieval/conversion of the vena cava filter;
- delivery systems, providing that they comprise an integral component of the deployment of the vena cava filter;
- optional filters that can be retrieved or converted, and permanent filters together with their associated endovascular systems. While this part of ISO 25539 might be useful with respect to the evaluation of repositioning filters after chronic implantation, it does not specifically address filter repositioning.

The following are outside the scope of this part of ISO 25539:

- temporary filters (e.g. tethered) that need to be removed after a defined period of time;
- coatings, surface modifications, and/or drugs;
- issues associated with viable tissues and non-viable biological materials;
- degradation and other time-dependent aspects of absorbable materials;
- procedures and devices (e.g. venous entry needle) used prior to the vena cava filter procedure.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10993 (all parts), Biological evaluation of medical devices

ISO 11135-1, Sterilization of health care products — Ethylene oxide — Part 1: Requirements for development, validation and routine control of a sterilization process for medical devices

ISO 11137-1, Sterilization of health care products — Radiation — Part 1: Requirements for development, validation and routine control of a sterilization process for medical devices

ISO 11607-1, Packaging for terminally sterilized medical devices — Part 1: Requirements for materials, sterile barrier systems and packaging systems

ISO 14630, Non-active surgical implants — General requirements

ISO 14937, Sterilization of health care products — General requirements for characterization of a sterilizing agent and the development, validation and routine control of a sterilization process for medical devices

ISO 14971, Medical devices — Application of risk management to medical devices

ISO 17665-1, Sterilization of health care products — Moist heat — Part 1: Requirements for the development, validation and routine control of a sterilization process for medical devices

# 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14630 and the following apply.

#### 3.1

#### access site

vein that is used for accessing the vena cava

EXAMPLE Jugular vein; femoral vein; subclavian vein; antecubital vein.

#### 3.2

#### adverse event

clinical event

complication, failure or device-related observation with preclinical *in vivo* and clinical use of the endovascular system or endovascular retrieval/conversion system

NOTE 1 This term relates to the definition of a hazardous situation that might lead to harm, as found in ISO 14971, when the consequences are to the patient.

NOTE 2 A clinical event might lead to a detrimental clinical effect.

#### 3.3

#### conversion system

component of the endovascular conversion system that is intended to structurally alter an optional filter after implantation so that it no longer functions as a filter

### 3.4

#### delivery system

component of the filter system, excluding the sheath/dilator, used to deliver the filter to the targeted position and to deploy the filter

NOTE The delivery system is removed after filter placement.

# 3.5

#### determine

requirement to quantitatively appraise or analyze

NOTE Also see evaluate (3.9).

## 3.6

#### detrimental clinical effect

discernible negative effect due to an adverse event or device failure

NOTE Descriptions of potential device effects of failure and failure modes and of detrimental clinical effects are given in Annex B.

#### 3.7

### endovascular filter system

filter system and sheath/dilator kit

See Figure 1.

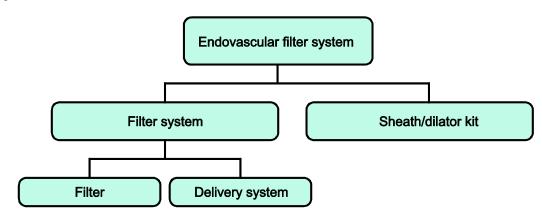


Figure 1 — Example of endovascular filter system

#### 3.8

#### endovascular retrieval/conversion system

retrieval/conversion system and sheath/dilator kit

See Figure 2.

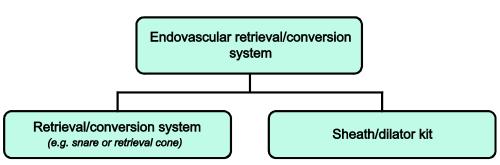


Figure 2 — Example of endovascular retrieval/conversion system

NOTE The term retrieval/conversion is used to describe either the retrieval or the conversion system and does not imply that one system can be used for both purposes.