

---

---

**Cosmetics — Analytical methods —  
Development of a global approach  
for validation of quantitative  
analytical methods**

*Cosmétiques — Méthodes analytiques — Développement d'une  
approche globale pour la validation des méthodes analytiques  
quantitatives*





**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Fax: +41 22 749 09 47  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
<b>Foreword</b> .....	<b>v</b>
<b>Introduction</b> .....	<b>vi</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms, definitions and symbols</b> .....	<b>1</b>
3.1 Terms and definitions.....	1
3.2 Symbols.....	5
<b>4 General principles</b> .....	<b>6</b>
4.1 Reminder.....	6
4.2 Various conditions for the estimation of precision.....	6
4.3 Accuracy profile.....	7
<b>5 Procedure</b> .....	<b>9</b>
5.1 Definition of the measured quantity.....	9
5.2 Definition of objectives.....	9
5.2.1 Choice of the scope of validation.....	9
5.2.2 Choice of acceptance limits.....	9
5.3 Selection of validation samples.....	10
5.3.1 Choice of the type of matrix or types of matrices.....	10
5.3.2 Methods for establishing reference values.....	10
5.4 Characterization plan for validation.....	10
5.4.1 Organization.....	10
5.4.2 Choice of the number of series, repetitions and concentrations for the characterization plan for validation.....	11
5.5 Calibration plan for the indirect methods.....	11
5.5.1 Organization.....	11
5.5.2 Choice of the number of series, repetitions and concentrations for the calibration plan.....	12
5.6 Testing.....	13
5.7 Calculation of predicted inverse concentrations for indirect methods.....	14
5.7.1 General.....	14
5.7.2 Calculation of the calibration models.....	14
5.7.3 Calculation of back-calculated concentrations by inverse prediction.....	15
5.8 Calculation of the validation criteria by concentration level.....	15
5.8.1 General.....	15
5.8.2 Trueness criteria by series.....	15
5.8.3 Trueness and precision criteria by concentration.....	16
5.8.4 Calculation of the tolerance intervals.....	17
5.9 Construction of the accuracy profile.....	18
5.10 Interpretation of the accuracy profile for validation.....	19
5.10.1 General.....	19
5.10.2 Decision rules.....	20
5.10.3 Definition of the scope of validity.....	21
5.10.4 Choice of a calibration procedure for the routine.....	21
5.10.5 Influence and significance of the $\beta$ proportion.....	21
5.10.6 Identification of outliers.....	22
<b>6 Management of the outcomes during routine use</b> .....	<b>22</b>
<b>Annex A (normative) Calculation of repeatability, intermediate precision and reproducibility standard deviations</b> .....	<b>23</b>
<b>Annex B (normative) Contents of the validation file</b> .....	<b>25</b>
<b>Annex C (informative) Setting-up an assay for determining the accuracy profile in the case of NDELA in cosmetic samples</b> .....	<b>27</b>

<b>Annex D (informative) Influence of the value of <math>\beta</math> on the tolerance interval (<math>R = 3</math> and <math>s_{IP} = 1</math>)</b> .....	<b>37</b>
<b>Annex E (informative) Contribution to the uncertainty calculation</b> .....	<b>38</b>
<b>Bibliography</b> .....	<b>39</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 217, *Cosmetics*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).


## Introduction

The purpose of this document is to propose a characterization protocol for the validation of a quantitative analysis method in the cosmetic field and thus responds to the requirements of ISO/IEC 17025, i.e. using the performance goals as a basis. The theoretical principles of this approach can be found in Reference [1]. This document is based on the French Standard NF V 03-110[2].

Analytical methods for analyses of cosmetics need to be validated. Validation has been long considered as a process consisting in individually verifying several different criteria, i.e. selectivity, repeatability, linearity, trueness, etc. The global approach, as proposed since 2003[1], is based on the total error concept and the term “global” means that only a single criterion should be checked to validate a method: the agreement between a future experimental result and the true value. This approach has already been applied in the domains of pharmacy[1],[9], agricultural chemistry[2], and is in agreement with quality assurance guidelines such as GLP or ISO/IEC 17025. This validation process applies generally to already developed methods and includes evaluations of the following criteria: specificity/selectivity, precision, trueness, linearity range, LOD/LOQ, stability, ruggedness.

The large number of cosmetic products and the variety of matrices present a challenge for an analytical laboratory requiring that standardized methods to be adapted for each type of samples. Additional difficulties are linked to the very low concentrations to be measured, generally of the order of the mg/kg (ppm) or µg/kg (ppb). In such context, criteria such as accuracy and uncertainty of measurement of the analytical results are of utmost importance.

When the concentration of a substance is determined by an analytical laboratory, it is important to evaluate the gap between the measured value and the known true value. This difference indicates the trueness of the analysis. If cosmetic samples are analysed several times in different conditions (laboratory, instrument, operator), the individual results will present a dispersal around the average value which represents the precision of the measurement. As for the individual measurement, it represents an error with the average value and an inaccuracy with regard to the reference value (i.e. the true value).

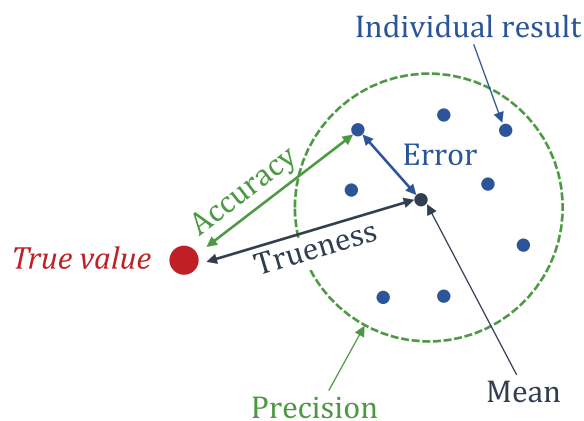


**Figure 1 — Illustration of the concepts of accuracy, precision and trueness**

When a laboratory measures the concentration of a given substance in a cosmetic product sample, the value which is obtained is thus characterized by a given accuracy which includes at the same time the notion of trueness and precision (see Figure 1). It can also be considered as total error. The insurance that the accuracy of a result is below acceptable limits, is thus one of the ways to make sure of the validity of a measurement.

The accuracy profile (plot of accuracy versus concentration), such as it is developed in numerous domains[3] to [9], is thus the way to know the accuracy on a result obtained with a given method applied to a type of sample in the environment of a given laboratory.

To reach this accuracy profile, it is necessary to undergo a specific assay allowing to demonstrate the validity of the analytical method, as well as the accuracy of the measurement for a given substance. In this approach, it is necessary to determine a tolerance interval<sup>[10]</sup> which contains a given proportion ( $\beta$ ) of future measured values inside (in average). If this tolerance interval is located inside a limit of acceptability defined a priori, taking into consideration several parameters such as the type and concentration of analyte, type of matrix, of analysis and conditions of the experiments, in this case, the method will be considered as valid, and if it goes outside this limit of acceptability, the method will be considered as non-valid (see [Figure 2](#)).

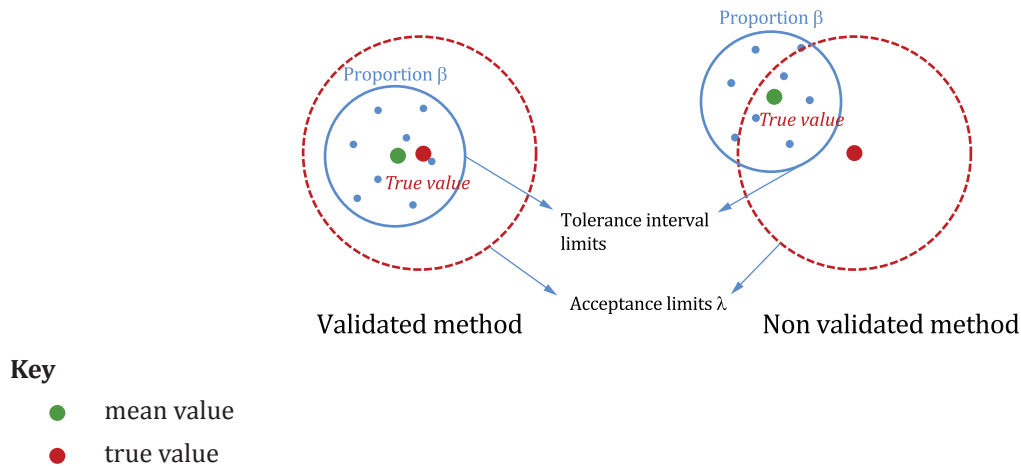

**Figure 2 — Illustration of the validation principle**





# Cosmetics — Analytical methods — Development of a global approach for validation of quantitative analytical methods

## 1 Scope

This document defines a global approach for the validation of a quantitative analytical method, based on the construction and interpretation of an accuracy profile, and specifies its characterization procedure.

This procedure is particularly applicable for internal validation in a cosmetic testing laboratory, but its scope can be extended to the interpretation of data collected for an interlaboratory study designed according to the recommendations of the ISO 5725-1. It does not apply to microbiological trials. The present approach is particularly suited to handle the wide diversity of matrices in cosmetics. This document only applies to already fully-developed and finalized methods for which selectivity/specificity have already been studied and the scope of the method to be validated has already been defined, in terms of matrix types and measurand (for example analyte) concentrations.

## 2 Normative references

The following document is referred to in the text in such a way that some or all of its content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO/IEC Guide 99:2007, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

## 3 Terms, definitions and symbols

### 3.1 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO/IEC Guide 99 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

#### 3.1.1

##### **measurement**

process of experimentally obtaining one or more quantity values that can reasonably be attributed to a quantity

[SOURCE: ISO/IEC Guide 99:2007, 2.1, modified — Notes to entry have been excluded.]

#### 3.1.2

##### **measurand**

quantity intended to be measured

Note 1 to entry: The term “analyte”, employed in chemistry, is a synonym of measurand, and is used more generally.

[SOURCE: ISO/IEC Guide 99:2007, 2.3, modified — Original notes to entry have been excluded and a new note to entry has been added.]